
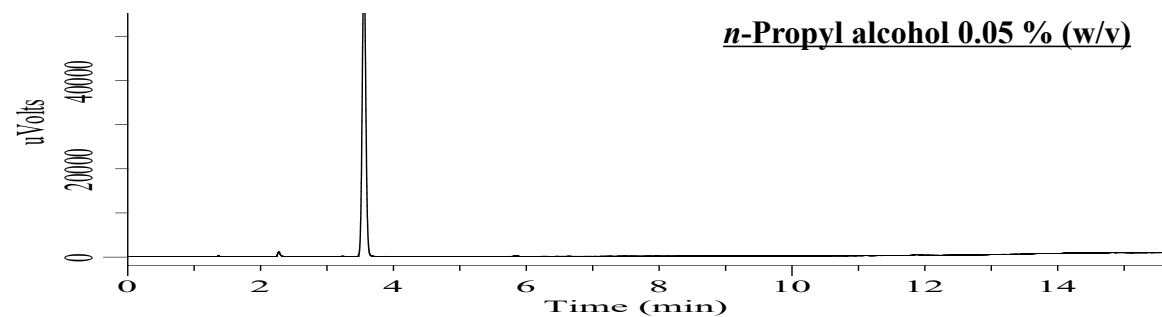
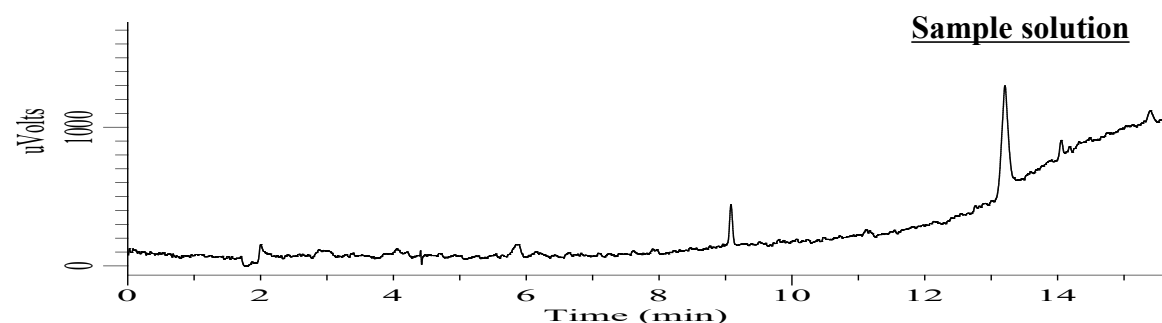


Analysis of Dextran 40

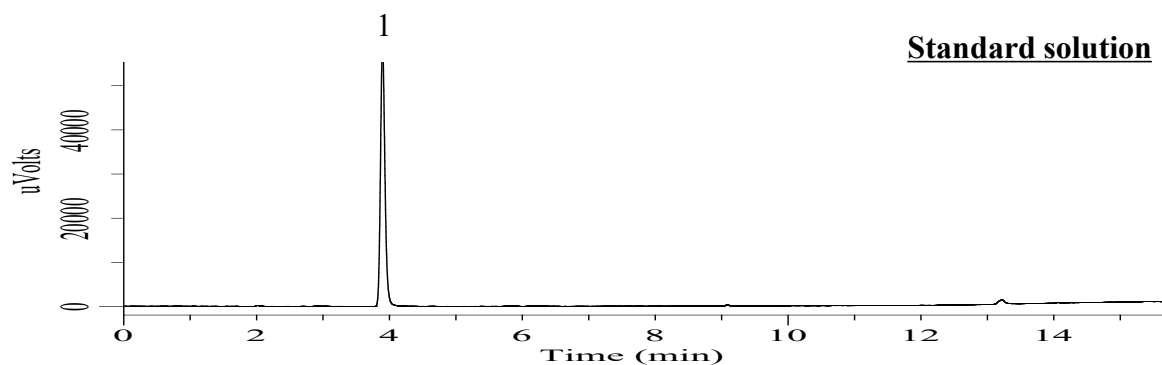

Conditions

System : GC-4000 Plus /FID
Column : InertCap 1 (GL Sciences Inc.)
 0.32 mm I.D. x 30 m df = 5.0 μ m
Col. Cat. No. : 1010-11249
Col. Temp. : 75 °C (4 min) - 15 °C/min - 220 °C (2 min)
Carrier Gas : N₂ 2 mL/min , Constant Flow
Injection : Split 1 : 10
 240 °C
Detection : FID Auto Range
 210 °C
Sample : Sample
 Standard
n-Propyl alcohol
Sample Size : 1 μ L

Analyte

1. *n*-Propyl alcohol 0.05 % (w/v)

Referenced to the Condition of the draft USP PF 50(4) Dextran 40.